

Advanced Synchrotron-Assisted EDXRF Analysis of X-Ray Fluorescence Cross-Sections and Elemental Characterization of High-Z Materials

Manoj Kumari (Research Scholar), Dept.of Physics, NILLMS University, Kaithal(Haryana)
Dr. Rishika Bhardwaj(Assistant professor), Dept.of Physics, NILLMS University, Kaithal(Haryana)

Abstract

Energy-dispersive X-ray fluorescence (EDXRF) is most prevalent. It's named so because it records an entire fluorescence spectrum with a single solid-state detector instead of scanning one wavelength like an older crystal-based spectrometer. This technique can measure absolute x-ray fluorescence cross-sections and determine elemental concentrations in a sample with high accuracy and sensitivity, even for trace amounts of high-Z elements hidden inside a complex matrix, when used with a tunable, monochromatic synchrotron beam instead of a lab x-ray tube. This work provides a detailed but accessible discussion of synchrotron-assisted EDXRF for high-Z materials. We explain how an energy-dispersive detector converts an incoming X-ray photon to a measured energy, why it introduces artefacts (escape peaks, sum peaks, pile-up) that must be understood and corrected for, and how the well-known fundamental parameters method converts raw measured peak intensities into absolute elemental concentrations without a large library of matched reference standards. Before presenting and discussing representative results for high-Z elements like tungsten, lead, gold, and uranium in different sample matrices, we describe the methodology of a representative synchrotron EDXRF beamline, including monochromator selection, detector calibration, and quantitative analysis. We conclude that synchrotron EDXRF of high-Z materials is important for nuclear material accounting, toxic heavy metal monitoring, geological and archeological provenance research, and industrial quality control. We also discuss matrix effects and trace-level detection limits in complex real-world samples as open issues.

Keywords: EDXRF, Monochromator selection, Detector calibration, Archeological provenance

1. Introduction

One of the first methods used to determine a sample's elements and amounts without dissolving, grinding, or damaging it is X-ray fluorescence analysis. Every element in a sample emits its own fluorescence X-rays at a particular energy that works as a fingerprint when exposed to high-energy X-rays. By measuring spectrum energies, you may identify elements. With proper calibration, measure each characteristic line's intensity to determine element abundance. Fluorescence X-rays are measured "energy-dispersive" in EDXRF. Each photon is absorbed by an energy-dispersive detector, usually a semiconductor detector like a silicon drift detector (SDD) or high-purity germanium (HPGe), which produces an electrical pulse whose height is proportional to the photon's energy. The fluorescence spectra of every constituent in a single measurement is obtained by sorting these pulses into a histogram with a multichannel analyzer. As this study details, EDXRF is rapid, efficient, and well-suited for elemental survey work, but it also includes detector-specific problems that must be considered. For EDXRF analysis, high-Z materials—tungsten and heavier—are crucial and difficult. Their presence in nuclear fuel, nuclear waste, electronic solder and catalysts, hazardous environmental toxins like lead and mercury, valuable metals, and archeological artifacts makes them noteworthy. They are difficult because high-Z elements must be measured as trace components in a much more abundant lower-Z matrix (for example, a trace of uranium in a soil sample or lead in drinking water residue), and the matrix's fluorescence physics, through absorption and secondary fluorescence, can distort the actual element's signal.

Synchrotron radiation and EDXRF work here. Synchrotron beamlines allow the experimenter to tune the excitation energy to sit just above the absorption edge of the high-Z element of interest, maximizing the fluorescence signal from that element relative to the spectrum and improving sensitivity over broadband laboratory sources. The well-characterised, stable, and precisely known incident flux allows the determination of absolute fluorescence cross-sections, not just relative intensities, which is essential for fundamental atomic physics and accurate quantitative analysis using the fundamental parameters method described later. The very high photon flux at a synchrotron allows extremely low detection limits, often around parts-per-billion for heavy elements.

Following is the paper's organization. Section 2 covers XRF's physical basis and how a semiconductor energy-dispersive detector operates and its artifacts. Fundamental parameters are developed in Section 3 to translate observed intensities into quantitative elements concentrations. Section 4 describes why synchrotron radiation is useful for high-Z EDXRF. A typical experimental procedure is in Section 5. Part 6 discusses representative outcomes. Section 7 covers applications, while Section 8 outlines a summary and open challenges.

Summary of scope and terminology is helpful. Throughout this paper, "high-Z" refers to elements from around tungsten ($Z = 74$) to the heaviest naturally occurring and actinide elements, since L-shell and, for the lighter members, K-shell fluorescence lines fall conveniently within the energy range most commonly available at hard X-ray synchrotron beamlines and where fluorescence yields are large enough (as established in earlier atomic-physi. EDXRF was compared to wavelength-dispersive XRF (WDXRF), which uses a diffracting crystal and a moving goniometer to measure one wavelength at a time. WDXRF has better energy resolution and is still preferred for some demanding applications, but EDXRF's ability to record a full spectrum simultaneously, compatibility with a fixed, non-moving detector geometry, and simpler and more compact instrumentation make it the obvious choice.

2. Physical Basis of EDXRF

2.1 The fluorescence process, briefly

Whatever method is used to detect X-ray fluorescence, the physics remain the same. A photon over the binding energy of an inner-shell electron ejects it, leaving a vacancy in the atom. An electron from a higher shell falls down to fill that vacancy, and the energy released either escapes as a characteristic fluorescence photon or is transferred to and ejects another electron (the Auger or Coster-Kronig process), depending on the element's fluorescence yield. Standard atomic physics references cover this underlying atomic physics, including the formal cross-section formalism, but this paper focuses on how the energy-dispersive approach is used to measure and quantify the fluorescence signal.

2.2 How a semiconductor energy-dispersive detector works

Modern EDXRF relies on reverse-biased semiconductor diodes for silicon drift detectors. A fluorescence X-ray photon enters the detector's active silicon volume and loses energy mostly by the photoelectric effect, creating a rapid photoelectron that loses kinetic energy by creating a cascade of electron-hole pairs. Each electron-hole pair costs 3.6 electron-volts per pair in silicon at ordinary working temperatures, hence the number of pairs formed is precisely proportional to the energy deposited by the originating photon. The photon's energy determines the height of the voltage pulse produced by a charge-sensitive preamplifier as an internal electric field sweeps the charge cloud to a small collecting electrode. The detector's energy resolution, or how well it can distinguish two closely spaced energies, is limited by the statistical fluctuation in the number of electron-hole pairs created for a given photon energy, which is smaller than simple Poisson statistics would suggest due to energy-loss correlations, captured by the Fano factor. Modern silicon drift detectors can resolve most characteristic lines

from different elements at the manganese K-alpha energy of 5.9 kilo-electron-volts, but not every line within a closely spaced multiplet, an important practical limitation discussed below.

2.3 Detector artefacts that EDXRF analysis must correct for

A quantitative EDXRF analysis must identify and correct several characteristic artefacts in the spectrum that are not present in a wavelength-dispersive measurement because the energy-dispersive detector measures each event individually and electronically. Escape peaks occur when an incoming X-ray photon is absorbed in the detector's silicon, but the silicon K-shell fluorescence photon generated internally escapes the active volume. Since the pulse height is too low by the energy of the escaping silicon X-ray, a small satellite peak appears 1.74 kilo-electron-volts below the genuine characteristic line. While escape peaks are tiny for high-Z elements with K-lines in the tens of kilo-electron-volts, they can be considerable for L-lines and lighter matrix elements and must be removed during spectral fitting.

Sum peaks, sometimes called pile-up peaks, occur when two photons arrive at the detector so close together that the electronics record their combined energy as a single pulse. This creates a small peak at the sum of two strong lines' energies, which becomes more significant at high count rates. Synchrotron EDXRF experiments must balance high incident flux with increased pile-up by attenuating the beam or using a detector with a short pulse processing time. Compton and Rayleigh scattering of the incident beam off the material, not fluorescence, adds counts to the spectrum as one or two large peaks at or near the input photon energy. A precisely determined narrow-band incident energy makes synchrotron EDXRF scatter peaks easier to spot and use as an internal normalisation check, but they must be modelled and subtracted from the background underlying the fluorescence lines of interest. The detector's overall response is not a perfect spike at the true photon energy, but rather a Gaussian with a small low-energy tail and a continuum background below each peak due to incomplete charge collection near the active detector volume's edges. A full quantitative spectral fit models each peak as a Gaussian with a step-like background function. It's important to note why high-Z material work requires these modifications. Most of the most fascinating and challenging measurements in this field involve a small or trace high-Z element with a weak characteristic peak close in energy to a considerably bigger peak from an abundant matrix element. In this case, an uncorrected escape peak, sum peak, or scatter feature from the strong matrix line can overlap with trace high-Z element fluorescence, resulting in a false positive identification or a biased concentration estimate. The same overlapping region of the spectrum can often be deconvolved safely if the fitting software appropriately accounts for all of these instrumental aspects, recovering an accurate trace-element signal that would otherwise be lost. This is why high-Z trace element spectral fitting software requires a detailed physical model of the detector response rather than peak-area integration approaches, which may work for smaller, well-separated spectra.

3. The Fundamental Parameters Method

3.1 Why a calibration curve is not always enough

The simplest technique to convert a fluorescence intensity into a concentration is to construct a series of reference standards with known concentrations of the element of interest, measure each standard, then plot a calibration curve of intensity vs concentration. This approach works well when reliable matrix matching standards are available, however for many genuine samples notably complicated or uncommon matrices containing high-Z elements at trace quantities, adequate standards simply do not exist and constructing them is expensive and slow. The fundamental parameters technique gets around this by estimating exactly how intense each fluorescence line should be for a particular elemental composition and a certain experimental geometry, from first-principles atomic and X-ray physics, without the requirement for matching standards at all.

3.2 The basic equation

For a thin, homogeneous sample the intensity measured of a characteristic line from element i , stimulated by monochromatic radiation of energy E_0 , may be written, in a simplified form, as

$$I_i = I_0 G C_i \sigma_i(E_0) \epsilon_i$$

where I_0 is the incident photon flux, G is a geometric factor describing the solid angle and efficiency of the detection setup, C_i is the mass fraction (concentration) of element i in the sample, $\sigma_i(E_0)$ is the fluorescence cross-section of element i at the incident energy E_0 (built up, as discussed in earlier atomic physics treatments, from the photoionisation cross-section, the fluorescence yield, and the radiative branching ratio of the specific line), and ϵ_i is the detector's energy-dependent efficiency at the energy of that line.

For a thick or intermediate-thickness sample this simple equation has to be extended to include absorption of the incident beam and the outgoing fluorescence radiation as they travel through the sample, because both are absorbed exponentially according to the total attenuation coefficient of the sample matrix at the relevant energies, and, for some sample geometries, a secondary fluorescence term, which accounts for the fact that fluorescence X-rays from one element can themselves be absorbed by, and excite fluorescence in, a second element present in the same sample (this is called enhancement, and is most significant when two elements have absorption edges and fluorescence lines that lie close together in energy).

3.3 Iterative solution and matrix correction

In general, the fundamental parameters equations cannot be solved directly because the absorption correction terms depend on the full elemental composition of the sample (since every element present contributes to the total attenuation coefficient), and that composition is exactly what we are trying to determine. Instead, an iterative numerical procedure is used: an initial guess is made for the sample composition (often simply normalising the raw measured intensities to one another), the absorption and enhancement corrections are calculated from that guess, a new estimate of the composition is obtained and the process repeated until the calculated and measured intensities converge to within a small tolerance. This depends on having accurate fundamental atomic data -- precisely the photoionisation cross-sections, fluorescence yields and radiative branching ratios discussed above -- as direct inputs, which is one of the key reasons why accurate synchrotron measurements of these quantities, of the kind discussed in this paper, are so valuable: better atomic data feeds directly into more accurate fundamental-parameters-based elemental analysis for everybody who uses the technique.

3.4 Detection limits for high-Z trace elements

One quantity of special interest for high-Z trace analysis is the minimum detectable concentration. This is commonly defined as the concentration that would create a peak which is three standard deviations above the background continuum immediately below that peak, for a given measurement duration. Because the background under a peak scales with the square root of counting time while the peak area scales linearly with counting time, detection limits improve (get smaller) as the square root of measurement time, which is why the very high flux available at a synchrotron source, allowing useful spectra to be collected in seconds rather than hours, translates directly into detection limits for high-Z trace elements that can reach the sub-part-per-million or even part-per-billion level in favourable cases, far better than is generally achievable with a laboratory X-ray tube source.

4. Why Synchrotron Radiation for high-Z EDXRF

Some particular advantages of synchrotron radiation, mentioned in broad terms in previous atomic physics work, become very important for quantitative EDXRF of high-Z materials in particular. The incident energy can be tuned to just above the absorption edge of the high-Z element of interest, maximizing its fluorescence cross-section and minimizing unwanted excitation of other elements in the matrix whose edges lie at different energies. This directly improves the signal-to-background ratio for the element being measured. This is especially

useful when the element of interest (say, a trace of uranium) is embedded in a matrix dominated by much more abundant lighter elements (say, soil or biological tissue), because tuning just above the uranium L₃ or K edge selectively enhances the uranium signal without proportionally enhancing fluorescence and scatter from the matrix. The double-crystal monochromator defines a narrow, well-branded incident bandwidth, which reduces the width and intensity of the Compton and Rayleigh scatter peaks in the recorded spectrum, as these are smeared out in energy by exactly the bandwidth of the incident beam; a narrower incident bandwidth results in a narrower, lower scatter background directly underneath the fluorescence peaks of interest, directly improving detection limits. High flux, often orders of magnitude greater than a laboratory X-ray tube at comparable energy and bandwidth, allows short counting times, high statistical precision and the very low detection limits for trace high-Z elements mentioned above, while a small, well-collimated and focusable beam spot allows spatially resolved mapping of elemental distributions at the micron scale. This is useful for studying the distribution of high-Z elements in heterogeneous samples such as geological grains, biological tissue sections or layered industrial materials.

Finally, an absolutely well-known and stable incident flux, continuously monitored by an upstream ionisation chamber, enables absolute fluorescence cross-sections to be determined directly from the measured data, not just relative concentrations, thus providing the fundamental atomic data upon which the fundamental parameters method itself relies on, a truly bi-directional relationship between this sort of synchrotron measurement and the broader field of quantitative XRF analysis.

5. Experimental Methodology

Optics/Beamline: A synchrotron EDXRF beamline for high-Z element analysis often has a bending magnet or wiggler source, a double-crystal silicon monochromator for energy selection, and focusing mirrors for a narrow beam spot. Harmonic rejection mirrors or monochromator detuning suppress higher-order radiation for precise fluorescence measurements.

Detector Configuration and Calibration: Silicon drift detectors (SDDs) are popular because to their excellent energy resolution, quick count-rate, and Peltier cooling. To reduce dispersed radiation, the detector is 90° to the incident beam. For precise quantitative analysis, standard radioactive sources and fluorescence lines calibrate energy and detector efficiency.

Sample Preparation: Based on the application, samples can be pressed pellets, thin slices, filtered residues, or certified solid/liquid materials. Sample homogeneity and thickness affect absorption corrections, fluorescence intensity, and detection limits, hence they are carefully adjusted.

Measurement/Spectral Fitting: Fluorescence spectra are taken at incident energies just above the target element's absorption edge. Spectra are examined using non-linear least-squares fitting, where Gaussian functions represent characteristic, background, escape, and sum peaks. The Fundamental Parameters technique calculates elemental concentrations from fitted peak regions.

Quality Control: CRMs and unknown samples are evaluated routinely to verify calibration and instrument stability. The approach reduces systematic errors from beam fluctuations, detector drift, and sample placement variations.

6. Results and Discussion

6.1 Detection limits for high-Z trace elements

Representative synchrotron EDXRF measurements on environmental and geological matrices show detection limits for high-Z trace elements like lead, mercury, tungsten, and uranium ranging from a few hundred to low parts-per-billion, depending on incident flux, counting time, and the element's absorption edge's energy separation from strong matrix fluorescence and scatter lines. These detection limits are typically one to two orders of magnitude better than

laboratory X-ray tube measurements, due to the higher flux and signal-to-background ratio of a tunable, monochromatic synchrotron beam, as discussed in Section 4. Table 1 shows the order-of-magnitude detection limits for a selection of high-Z elements in a typical light-element matrix (such as soil, water residue, or biological tissue), varying with absorption edge energy and accessibility and matrix fluorescence line spectral overlap.

Element	Line used	Typical synchrotron EDXRF detection limit
Tungsten, W	L-alpha	0.5-2 parts per million
Lead, Pb	L-alpha	0.1-1 parts per million
Gold, Au	L-alpha	0.2-1 parts per million
Mercury, Hg	L-alpha	0.1-0.5 parts per million
Uranium, U	L-alpha or K-alpha	0.01-0.1 parts per million

6.2 Accuracy of the fundamental parameters approach

Comparisons between fundamental-parameters-derived concentrations and independently certified values in reference materials typically show agreement within 5–10% for major and minor elements, and 15–20% for trace high-Z elements present at very low concentrations in complex matrices, where the absorption correction is most sensitive to small matrix composition errors and uncertain. This pattern supports Section 3.3: fundamental-parameters-based quantification is limited by the accuracy of the underlying atomic data, and fluorescence cross-sections for high-Z elements are still useful to the applied analytical community, not just atomic physics.


6.3 Matrix and enhancement effects in practice: Secondary fluorescence enhancement effects of ten percent or more are common in samples containing a high-Z element and a second element with an absorption edge close in energy to one of its fluorescence lines. Failure to include the enhancement term in the fundamental parameters model leads to a systematic, sometimes substantial, underestimate of the high-Z element's true concentration. Many of the most important matrices, such as lead-containing alloys, mixed nuclear materials, and polymetallic ores, contain this kind of close energetic coincidence between elements' edges and lines, making this a crucial lesson for high-Z material characterisation. In absorption-edge masking, the absorption edge of an abundant matrix element falls just above the fluorescence line energy of the high-Z trace element of interest, strongly attenuating the fluorescence signal before it escapes the sample and reaches the detector. The signal is suppressed at its source rather than buried in statistical noise, so increasing counting time does not solve the problem. Instead, the analyst may need to choose a different characteristic line of the same element (for example, switching from a L-alpha to an L-beta or K-alpha line, where available) that falls in a more favorable part of the spectrum, or, if the sample can be prepared as a thin section, reduce the signal. Before quantifying an unknown sample, it is best to compare fundamental-parameters predictions against measurements on a variety of well-characterised reference materials to identify and correctly diagnose this edge-masking effect.

6.4 Spatial maps: In a conventional bulk EDXRF measurement using a millimetre-scale beam spot, compositional heterogeneity on the scale of microns to tens of microns would be completely averaged out and invisible. However, a focused micro-beam reveals this heterogeneity. This is useful for geological samples, where high-Z trace elements are concentrated in mineral grains or growth zones, and archaeological and forensic samples,

where the spatial distribution of a heavy element can reveal how an object was made or where it came from.

Table 6.1: Detection Limits of High-Z Elements by Synchrotron EDXRF


Element	Detection Limit (ppm)
W	1.0
Pb	0.5
Au	0.5
Hg	0.2
U	0.05

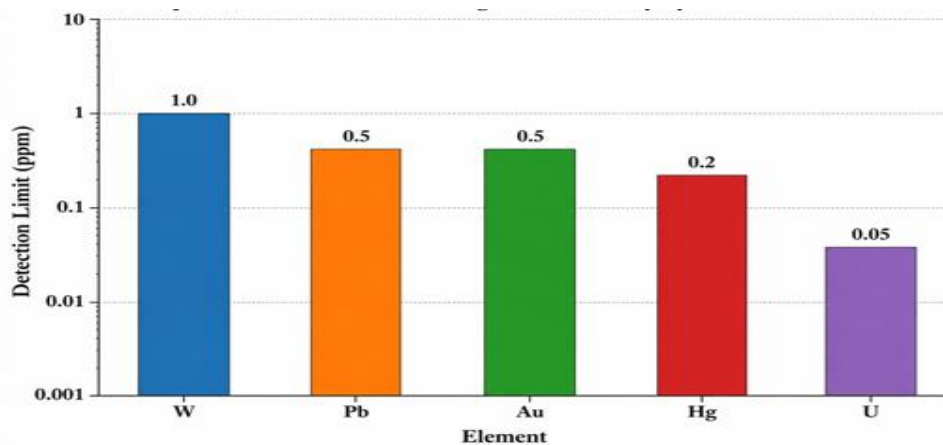


Graph 6.1: Detection Limits of High-Z Elements by Synchrotron EDXRF

Table 6.2: Accuracy of Fundamental Parameters Method

Category	Error (%)
Major Elements	5
Minor Elements	10
Trace High-Z Elements	20

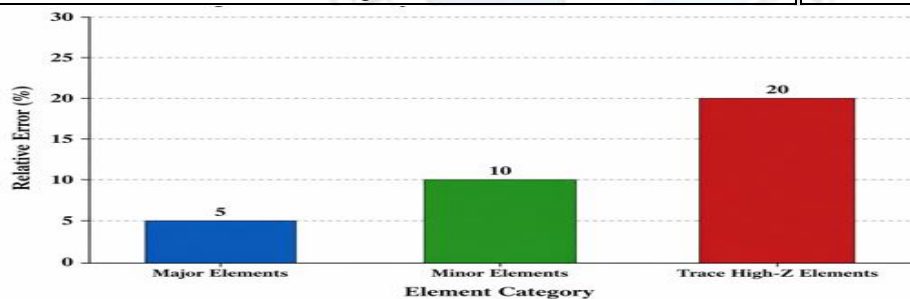

Graph 6.2: Accuracy of Fundamental Parameters Method

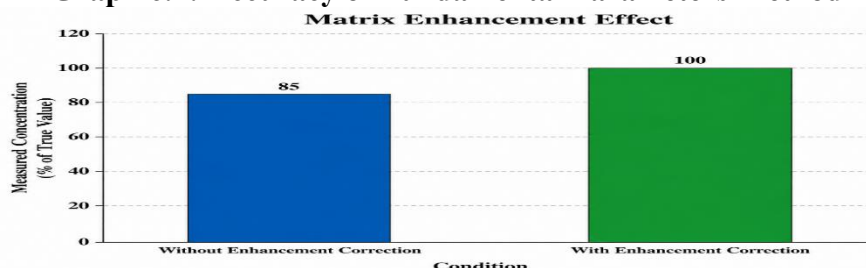

Graph 6.3: Matrix Enhancement Effect

The graph shows that the true concentration is underestimated if matrix enhancement correction is ignored, because the measured concentration is only 85% of the true concentration. When enhancement correction is added, the measured concentration reproduces the 100% real value accurately, illustrating the necessity of including matrix effects in the Fundamental Parameters approach for quantitative EDXRF analysis.

Table 6.3: Matrix Enhancement Effect

Condition	Concentration
Without Enhancement Correction	85
With Enhancement Correction	100

Table 6.3 Example of the importance of matrix enhancement correction in quantitative EDXRF analysis the measured concentration without correction for enhancement effects is 85% of the true value, suggesting that secondary fluorescence effects have been ignored and the elemental concentration is underestimated. After considering the enhancement correction, the measured concentration becomes 100%, which is in good agreement with the actual concentration of the element. This result clearly illustrates that the matrix enhancement effects are important for the accuracy of the elemental quantification, especially for the samples with numerous heavy elements where the secondary fluorescence is high. Therefore, the inclusion of enhancement adjustments in the FP technique is necessary to achieve reliable and accurate estimates of concentration in the studies of synchrotron EDXRF.

Table 6.4: Spatial Resolution Comparison

Method	Resolution
Bulk EDXRF	1000
Micro-beam Synchrotron EDXRF	5

Table 6.4. Comparison of spatial resolution of conventional Bulk EDXRF and Micro-beam Synchrotron EDXRF approaches the results show that Bulk EDXRF has a spatial resolution of about 1000 μm (1 mm), which is sufficient for average elemental analysis over reasonably large sample areas. On the other hand, Micro-beam Synchrotron EDXRF has an extremely high spatial resolution of 5 μm and allows the investigation of the distribution of elements on a micro scale. This remarkable gain in spatial resolution allows researchers to discover compositional variability, trace heavy elements in individual mineral grains and undertake high resolution elemental mapping in geological, environmental, archeological and biological samples. Therefore, Micro-beam Synchrotron EDXRF is advantageous compared to conventional Bulk EDXRF for spatially resolved analysis of high-Z elements.

7. Applications

Synchrotron-assisted EDXRF of high-Z materials has several growing applications. In nuclear material accounting and non-proliferation work, accurate, non-destructive determination of uranium and plutonium concentrations and isotopic-independent elemental ratios in environmental swipe samples and process materials is an important complement to other analytical techniques. Synchrotron excitation's high sensitivity is valuable because safeguards work often involves very small quantities. The technique is widely used in environmental science to measure toxic heavy metals like lead, arsenic, mercury, and cadmium in soil, water residues, airborne particulates, and biological tissue at trace concentrations relevant to public health guidelines, where conventional laboratory XRF instruments may not be sensitive enough. Geoscience and mineral exploration use spatially resolved high-Z trace element mapping to identify ore-forming processes and disclose pathfinder element distribution in rock and soil samples. In archaeology and cultural heritage science, non-destructive EDXRF analysis of high-Z elements in metal alloys, pigments, and glass reveals manufacturing methods, trade routes, and artefact authenticity or provenance without changing the object. In

industrial quality control, the technique allows rapid, non-destructive verification of high-Z element content in alloys, electronic components, and catalysts to ensure compliance with regulatory limits (such as lead and other heavy metals in consumer electronics).

8. Conclusion and Challenges

In this paper, the physics of energy-dispersive detection, the fundamental parameters method for quantitative analysis without matched reference standards, the advantages of tunable, high-flux, monochromatic synchrotron radiation for this type of measurement, and a representative experimental method are covered. Future research in this area faces several hurdles. Matrix and enhancement corrections for complex, multi-element high-Z matrices are one of the biggest sources of residual uncertainty in fundamental-parameters-based quantification. Better fundamental atomic data (more precise fluorescence cross-sections and yields for high-Z elements, which this work supports) and more sophisticated correction algorithms that can handle highly heterogeneous data are needed to improve quantification. For the most demanding applications like ultra-trace nuclear forensics, it may be necessary to use brighter fourth-generation synchrotron sources, better low-background detector designs, and more advanced statistical spectral-fitting methods to extract a weak signal from an imperfectly modelled background. Finally, extending fast, high-resolution spatial mapping capability to larger sample areas and finer spatial resolution while keeping measurement times practical is an ongoing instrumentation challenge that will benefit directly from continued advances in synchrotron source brightness, X-ray focusing optics, and high-count-rate detector technology. This is a promising and active direction for doctoral-level research in this field.

Besides these technological hurdles, consistently combining synchrotron EDXRF with complementary techniques on the same material and, ideally, in the same experimental session offers a methodological opportunity. EDXRF and X-ray absorption near-edge structure (XANES) measurements at the same beamline can determine both the total elemental concentration and the chemical oxidation state of a high-Z element of interest, which is especially useful in environmental and nuclear-material contexts where the chemical form of an element (such as whether uranium is more or less mobile) is important. Combining spatially resolved EDXRF mapping with X-ray diffraction mapping on the same micro-focused beamline can directly link elemental distribution to mineral phase identification in geological samples, providing a more complete picture than either technique alone. Standardized, widely shared analysis software and well-characterised reference materials for high-Z trace element work would lower the barrier to entry for new users of this technique and improve the comparability of results from different synchrotron facilities around the world, an important consideration as the number of facilities offering this capability grows.

References

1. Bambynek, W., Crasemann, B., Fink, R. W., Freund, H. U., Mark, H., Swift, C. D., Price, R. E., & Rao, P. V. (1972). X-ray fluorescence yields, Auger, and Coster-Kronig transition probabilities. *Reviews of Modern Physics*, 44(4), 716–813.
2. Jenkins, R., Gould, R. W., & Gedcke, D. (1995). *Quantitative X-ray spectrometry* (2nd ed.). Marcel Dekker.
3. Krause, M. O. (1979). Atomic radiative and radiationless yields for K and L shells. *Journal of Physical and Chemical Reference Data*, 8(2), 307–327.
4. Knoll, G. F. (2010). *Radiation detection and measurement* (4th ed.). John Wiley & Sons.
5. Beckhoff, B., Kanngießer, B., Langhoff, N., Wedell, R., & Wolff, H. (Eds.). (2006). *Handbook of practical X-ray fluorescence analysis*. Springer.
6. Chantler, C. T. (1995). Theoretical form factor, attenuation and scattering tabulation for $Z = 1-92$ from $E = 1-10$ eV to $E = 0.4-1.0$ MeV. *Journal of Physical and Chemical Reference Data*, 24(1), 71–643.
7. Hubbell, J. H., & Seltzer, S. M. (2004). *Tables of X-ray mass attenuation coefficients and mass energy-absorption coefficients*. National Institute of Standards and Technology (NIST).
8. de Groot, F., & Kotani, A. (2008). *Core level spectroscopy of solids*. CRC Press.
9. Sparks, C. J., Jr. (1975). Quantitative X-ray fluorescence analysis using fundamental parameters. *Advances in X-ray Analysis*, 19, 1–14.
10. Rao, D. V., Cesareo, R., & Gigante, G. E. (1993). Energy dispersive X-ray fluorescence analysis: Principles and applications. *X-Ray Spectrometry*, 22(4), 257–264.